

# Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test

## INSTRUCTIONS FOR USE

REF GCFC-525SKa-H1/GCFC-525SKa-H2/GCFC-525SKa-H4

### IVD

For Over The Counter Use  
For *in vitro* diagnostic use

### INTENDED USE

The Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test is a lateral flow immunochromatographic assay intended for the qualitative detection and differentiation of influenza A, and influenza B nucleoprotein antigens and SARS-CoV-2 nucleocapsid antigen directly in anterior nasal swab samples from individuals with signs and symptoms of respiratory tract infection. Symptoms of respiratory infections due to SARS-CoV-2 and influenza can be similar. This test is for non-prescription home use by individuals aged 14 years or older testing themselves, or adults testing individuals aged 2 years or older.

All negative results are presumptive and should be confirmed with an FDA-cleared molecular assay when determined to be appropriate by a healthcare provider. Negative results do not rule out infection with influenza and SARS-CoV-2 or other pathogens. Individuals who test negative and experience continued or worsening respiratory symptoms, such as fever, cough and/or shortness of breath, should therefore seek follow-up care from their healthcare provider.

Positive results do not rule out co-infection with other respiratory pathogens and therefore do not substitute for a visit to a healthcare provider or appropriate follow-up.

### SUMMARY

COVID-19 and influenza are acute and highly contagious viral infections of the respiratory tract. The causative agents of the diseases are immunologically diverse, single-strand RNA viruses known as SARS-CoV-2 viruses and influenza viruses, respectively. There are three types of influenza viruses: A, B and C. Type A viruses are the most prevalent and are associated with more serious disease whereas Type B infection is generally milder. Type C virus has never been associated with a large epidemic of human disease.

A patient can be infected with a single virus or co-infected with SARS-CoV-2 and one or more types of influenza viruses. These viral infections occur more often during the respiratory illness season (in the U.S. this includes the fall and winter seasons) and the symptoms generally appear 3 to 7 days after the infection. Transmission for all of these viruses occurs through coughing and sneezing of aerosolized droplets from infected people, who may be either symptomatic or asymptomatic. For symptomatic patients, the main symptoms include fever, fatigue, dry cough, and loss of taste and smell. Nasal congestion, runny nose, sore throat, myalgia, and diarrhea were also associated symptoms.

Rapid diagnosis of SARS-CoV-2 and influenza A & B viral infection will help healthcare professionals treat patients and control these diseases more effectively.

### PRINCIPLE

The Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test is an immunochromatographic assay that uses highly sensitive monoclonal antibodies to detect nucleocapsid protein antigens extracted from COVID-19, influenza virus types A and B with anterior nares swab samples.

The test device is a plastic housing, known as a cassette, containing two test strips, each composed of the following parts: sample pad, reagent pad, reaction membrane, and absorbing pad. The reagent pads contain colloidal gold conjugated with monoclonal antibodies (mAb) specific for SARS-CoV-2, Influenza A, and Influenza B target proteins. When the test sample is added into the sample well (S) of the cassette, mAb conjugates dried in the reagent pad are dissolved and interact with the viruses' proteins in the sample (if present). These complexes migrate along the test strip and across the reaction lines on the membrane. The reaction line contains a second antibody specific to available target protein-mAb complexes with each of the virus antigens of the test, resulting in visible test lines for the viruses in the sample.

Results completely develop after 15 minutes. Reactions for each virus occur independently at their respective locations on the test reaction membrane. If the sample contains influenza type A or B antigens, a pink-to-red test line (A or B) will develop; if SARS-CoV-2 antigens are present, a pink-to-red test line (T) will develop. The procedural control line (C) must always appear on both strips for the test to be valid. The Healgen® Rapid Check® COVID-19/Flu A&B Antigen test is validated for testing direct samples without transport media and does not use biotin-streptavidin/avidin chemistry in any of the steps for coupling reagents.

### WARNINGS, PRECAUTIONS, AND SAFETY INFORMATION

1. Read the instructions fully and carefully before performing the procedure. Failure to follow the instructions may result in inaccurate or invalid results.
2. **Do not use the test if you have had symptoms for more than 5 days or no symptoms at all.**
3. **Do not use under 2 years of age.**
4. Do not use the test kit after its expiration date.
5. Do not use the test if the pouch is damaged or open.
6. Do not reuse the test cassette, processing solution, or swab.
7. Not for use with viral transport media (VTM).
8. Do not open the test contents until ready for use. If the test cassette is open for an hour or longer, invalid test results may occur.
9. When collecting a sample, only use the swab provided in the kit.
10. Inadequate or inappropriate sample collection, storage, or transport may yield false test results.
11. Testing should be performed in an area with good lighting.
12. **Keep the testing kit and kit components away from children and pets before and after use. Avoid contact with your skin, eyes, nose, or mouth. Do not ingest any kit components. The reagent solution contains harmful chemicals (see table below). If the solution contacts your skin, eyes, nose, or mouth, flush with large amounts of water. If irritation persists, seek medical advice: <https://www.poisonhelp.org> or 1-800-222-1222.**

Hazard Category (mixture)	Hazard Class	GHS Hazard Statement for mixture	Hazardous Ingredients (%)*
2	Skin irritation	Causes skin irritation (H315)	Tris (2.4%) 1, 2-Benzisothiazolin-3-One (0.04%)
Hazard Category (mixture)	Hazard Class	GHS Hazard Statement for mixture	Hazardous Ingredients (%)*
2	Eye Irritation	Causes eye irritation (H320)	1, 2-Benzisothiazolin-3-One (0.04%) Tris (2.4%) Ethylenediamine ethoxylated propoxylated polymer (S9) (0.75%)

## STORAGE AND STABILITY

- Store the test kit between 36-86°F (2-30°C) in a place out of direct sunlight.
- Reagents and devices must be used at room temperature (59-86°F/15-30°C).
- The unsealed cassette is valid for 1 hour. It is recommended to use the test kit immediately after opening. The expiration date is on the package.

## MATERIALS PROVIDED

- 1/2/4 Sealed Test Cassette(s)
- 1/2/4 Sterile Nasal Swab(s)
- 1/2/4 Pre-filled Extraction Tube(s)
- 1/2/4 Extraction Tube Tip(s)
- 1 Tube Holder
- 1 Quick Reference Instructions (QRI)

## MATERIALS REQUIRED BUT NOT PROVIDED

- Timer or clock


## PREPARING FOR THE TEST

### NOTE:

- Do not open the test contents until ready for use. If the test cassette is open for an hour or longer, invalid test results may occur.
- Allow the test device and reagents to come to room temperature [15-30°C(59-86°F)] prior to testing.

### 1. Check the test's expiration date printed on the outer test packaging.

- Wash your hands with soap and water for 20 seconds and dry them thoroughly, or use hand sanitizer.
- Turn over the test kit box to locate the perforated hole.




- Insert the extraction tube into the tube holder. Ensure that the tube is stable and upright.
- Tear off the sealing film on the extraction tube gently to avoid spilling the liquid.
- Remove test cassette from sealed pouch and lay it on a flat surface.

## SAMPLE COLLECTION


- Remove the swab from the pouch. Carefully insert the sterile swab no more than 3/4 inch (1.5 cm) into the nostril.

**Note:** Be careful not to touch the swab tip (soft end) with hand.



- Slowly rotate the swab at least 5 times against the nostril wall for at least 15 seconds. Remove the swab and repeat in the other nostril using the same swab.

**Note:** If you are swabbing others, please wear a face mask. With children, the maximum depth of insertion into the nostril may be less than  $\frac{1}{2}$  to  $\frac{3}{4}$  of an inch, and you may require another adult to hold the child's head while swabbing

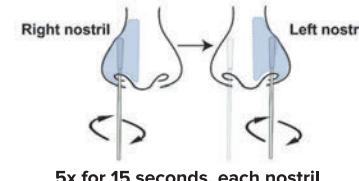


5x for 15 seconds, each nostril


## RUNNING THE TEST

- Immerse the swab into the pre-filled extraction tube and swirl the swab in the buffer. Ensure the sample is mixed thoroughly by making at least 6 circles.


**Note:** Sample must be mixed in the extraction buffer within 1 hour of sample collection



- Leave the swab in the extraction tube for 1 minute. A timer is recommended for this step.



- After 1 minute, pinch the tip of the swab from the outside of the tube to remove any excess sample in the swab. Remove and discard the swab.




6. Hold the tube upright and insert the extraction tube tip into the tube opening. Ensure a tight fit to prevent leaking.



7. Invert the extraction tube and **squeeze 8 drops** of test sample into the sample well. Then discard the tube.

**Note:** *Sample must be applied to the test cassette within one hour of completing step 3.*




8. Start timer. Read results between 15 minutes and 20 minutes.

**Note:** *Do not read the test results before 15 minutes or after 20 minutes as this can give false or invalid results.*



15 minutes

## INTERPRETING YOUR RESULTS



Control line = **C**  
Flu B line = **Flu B**  
Flu A line = **Flu A**

**C** = Control line  
**COVID** = COVID-19 line

- **Do not read test results before 15 minutes or after 20 minutes. Results read before 15 minutes or after 20 minutes may result in false or invalid results.**
- This test is using an internal procedural control that is needed to generate a valid result for your test. If a colored line appears in the control line regions (C) in the test window this confirms that membrane wicking has occurred and the test reagents are functional. A test result is valid when both strips have a visible control line.
- Look for lines next to 'C' (Control), 'Flu B', 'Flu A' and 'COVID'.
- Look closely! Any faint line is still a line.
- If uncertain how to proceed, contact Technical Assistance at support@healgen.com or (866) 982-3818 (Monday-Friday 8:30 a.m. to 5 p.m. CDT).

## Additional Information: Reading Results

**IMPORTANT:** Do not use the test as the only guide to manage your illness. Consult your healthcare provider if your symptoms persist or become more severe. Individuals should provide all results obtained with this product to their healthcare provider.






Scan QR code for more information on reading results.

Webpage: <https://www.healgen.com/covid19-influenza-a-b-OTC>

A paper version of the labeling can be obtained free of charge by contacting Healgen Customer Service at +1 (866) 982-3818 or at [support@healgen.com](mailto:support@healgen.com)

### Invalid test result



Check to see if a line is visible at the control line 'C' on both strips.




If you do not see any C line, or only see one C line, DO NOT CONTINUE reading the results. It means your test is invalid

**Note:** *The 3 images displayed are examples only; additional invalid outcomes are possible.*

An invalid test result means that the test is unable to determine if you are infected with influenza or SARS-CoV-2 (COVID-19) or not. The test needs to be repeated with a new kit and sample.

### Negative test result




**Both 'C' lines only**

If you do not see a line at 'COVID', 'Flu A' or 'Flu B' it means you may not have COVID-19, Flu A or Flu B virus.

If you still have COVID-19, Flu A or Flu B symptoms, you should seek follow up care with your healthcare provider.

A negative test result means that COVID-19, Flu A, and/or Flu B viruses were not detected in the sample. A negative result is presumptive because despite a negative result you may still have COVID-19, Flu A, and/or Flu B infection. This is because the amount of virus in your sample may be too low for the test to detect it, which is called a 'false negative result'. False negative results can occur if you read your test result before the 15 minutes have passed or when your sample has only a low amount of virus in it. Low amount of virus can occur if you take your sample at a time when your symptoms just started appearing, or when you already started to feel better at the end of your infection. If you tested negative and continue to experience COVID-19, Flu A, and/or Flu B-like symptoms, you should therefore seek follow-up care with your healthcare provider who will determine the best course of action. Your health care provider can also determine if confirmation of your test result with a molecular assay is necessary.

#### Positive test result

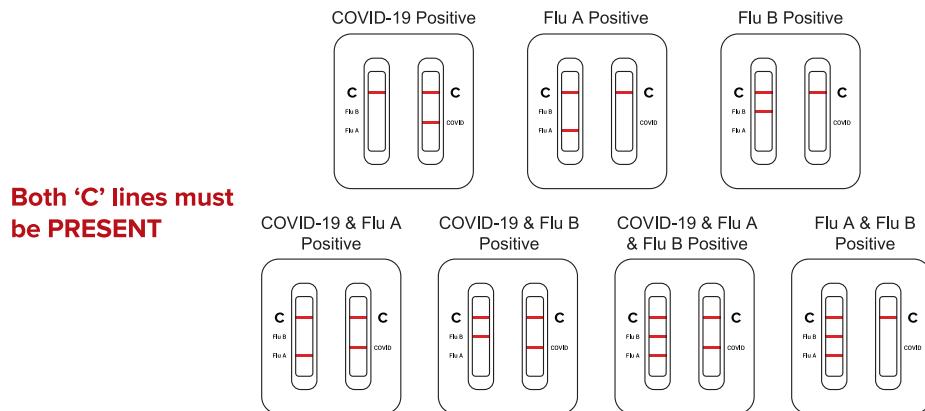

If you see a line at any one, or multiple, of the 'COVID', 'Flu A' or 'Flu B' areas, it means that your test result is positive and the virus annotated next to the positive line was detected in your sample. Consult your healthcare provider to discuss your positive test result. Self-isolate at home per CDC recommendations to stop spreading virus to others.

A positive test result means that any one, or multiple, of the viruses detected by this test were also detected in your sample. It is very likely that you have the respective COVID-19 or influenza infection(s) and are contagious. You should self-isolate following local guidelines. Please contact your physician or healthcare provider to discuss your tests results and follow-up care. In rare instances, individuals may also have co-infections with other bacteria or viruses that this test is not designed to detect. This means that the virus detected by this test may not be the definitive or the only cause of your disease. There is a very small chance that this test or influenza infection can give you a positive result that is incorrect (a false positive).

#### Reporting Your Results

Securely report your Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test result(s) at MakeMyTestCount.org by visiting: <https://makemytestcount.org/healgenscientific> – this voluntary and anonymous reporting helps public health teams understand COVID-19 spread in your area and across the country and informs public health decisions.



#### LIMITATIONS

- The clinical performance of this test was established based on the evaluation of a limited number of clinical specimens collected between February 2024 through April 2024. The clinical performance has not been established for all circulating variants but is anticipated to be reflective of the prevalent variants in circulation at the time and location of the clinical evaluation. There is a risk of false negative results due to the presence of novel, emerging respiratory virus variants. Test accuracy may change as new virus variants of COVID-19 and influenza emerge.
- This test provides a presumptive negative result; this means the test only provides preliminary results that should be confirmed using an independent, highly sensitive molecular test to make well-informed clinical decisions.
- A negative test result may occur if the level of antigen in the sample is below the detection limit of the test or if the sample is collected, handled or transported improperly.
- There is a higher chance of false negative results with antigen tests than with laboratory-based molecular tests due to the sensitivity of the test technology. This means that there is a higher chance this test will give a false negative result in an individual with COVID-19 as compared to a molecular test, especially in samples with low viral load.
- False positive test results are more likely when the prevalence of SARS-CoV-2, influenza A, and/or influenza B is low in the community.
- Positive results do not rule out co-infection with other respiratory pathogens.
- Persons with risk factors for severe disease from respiratory pathogens (e.g., young children, elderly individuals, chronic lung disease, heart disease, compromised immune system, diabetes, and other conditions) should contact a healthcare provider; users should also contact a healthcare provider if symptoms persist or worsen.
- This test is read visually and has not been validated for use by those with impaired vision or color-impaired vision.
- Incorrect test results may occur if a specimen is incorrectly collected or handled.
- This device is a qualitative test and cannot provide information on the amount of virus present in the specimen.
- This test detects both viable (live) and non-viable influenza A, influenza B, and SARS-CoV-2. Test performance depends on the amount of virus (antigens) in the sample and may or may not correlate with viral culture results performed on the sample.
- Exposure to hand sanitizer may cause false negative results with this test.
- Individuals who recently received nasally administered influenza A or influenza B vaccine may have false positive influenza test results after vaccination.
- This test does not distinguish between SARS-CoV and SARS-CoV-2.

## PERFORMANCE CHARACTERISTICS

A prospective study was completed at ten sites in the United States for clinical validation of the Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test for the detection of the SARS-CoV-2/Flu A/Flu B in self-collected anterior nasal (AN) swab samples. The study evaluated the Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test performance in symptomatic individuals who were currently experiencing symptoms associated with COVID-19, influenza A and/or influenza B. A total of 1156 subjects experiencing symptoms associated with COVID-19/Flu A/Flu B with symptom onset between 0 and 5 days were enrolled in the study. 1122 were evaluable, of which 1122 subjects were evaluable for Flu A/B, and 1097 were evaluable for SARS-CoV-2.

Each enrolled subject either self-collected a dual anterior nares (AN) sample or had a dual AN sample collected from him/her by another individual for the investigation test. Each subject also had a dual AN sample collected from him/ her by one of the study personnel for the comparator testing, which were FDA cleared RT-PCR assays. Swab collections for investigation and comparator samples were alternated by subject. The comparator tests were performed according to their respective instructions for use. Test results from the Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test were compared to the results generated from comparator tests. Results are shown in Tables 1.1-1.4.

**Table 1.1: Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test – Results for SARS-CoV-2**

SARS-CoV-2 Test Results	RT-PCR Comparator		
	Positives	Negatives	Total
Positives	69	10	79
Negatives	6	1012	1018
Total	75	1022	1097

Positive Percent Agreement = (69/75) = 92.0% (95% CI: 83.6% - 96.3%)

Negative Percent Agreement = (1012/1022) = 99.0% (95% CI: 98.2% - 99.5%)

**Table 1.2: SARS-CoV-2 Clinical Performance Stratified by Days Post Symptoms Onset (DPSO)**

DPSO	Total Number of Subjects	Healgen Test Positive	Comparator Positives	Positivity Rate by Comparator	PPA	95% CI
Day 0	24	0	0	0.0%	NA	
Day 1	180	12	13	7.2%	92.3%	66.7% - 99.6%
Day 2	341	15	17	5.0%	88.2%	65.7% - 96.7%
Day 3	285	16	17	6.0%	94.1%	73.0% - 99.7%
Day 4	194	21	21	10.8%	100.0%	84.5% - 100.0%
Day 5	73	5	7	9.6%	71.4%	35.9% - 91.8%
<b>Total</b>	<b>1097</b>	<b>69</b>	<b>75</b>	<b>6.8%</b>	<b>92.0%</b>	<b>83.6% - 96.3%</b>

**Table 1.3: Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test – Results for FLU A**

Flu A Test Results	RT-PCR Comparator		
	Positives	Negatives	Total
Positives	49	1	50
Negatives	4	1068	1072
Total	53	1069	1122

Positive Percent Agreement = (49/53) = 92.5% (95% CI: 82.1% - 97.0%)

Negative Percent Agreement = (1068/1069) = 99.9% (95% CI: 99.5% - 100.0%)

**Table 1.4: Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test – Results for FLU B**

Flu B Test Results	RT-PCR Comparator		
	Positives	Negatives	Total
Positives	38	1	39
Negatives	4	1079	1083
Total	42	1080	1122

Positive Percent Agreement = (38/42) = 90.5% (95% CI: 77.9% - 96.2%)

Negative Percent Agreement = (1079/1080) = 99.9% (95% CI: 99.5% - 100.0%)

## SUBJECT DEMOGRAPHICS

**Table 2: Subject Demographics of All Enrollments**

Demographic	Subjects (by lay-user collection and testing (N=178)	Self-collecting and testing (N=944)	Overall (N=1122)
Age: Mean (SD)	8.2 (6.0)	41.3 (15.9)	36 (19.1)
Age: Median [Min, Max]	8 [2, 71]	40 [14, 89]	35 [2, 89]
Age Group			
≥2 - <14 years of age	171 (96.1%)	0 (0.0%)	171 (15.2%)
≥14 - <24 years of age	6 (3.4%)	147 (13.1%)	153 (13.6%)
≥24 - <65 years of age	0 (0.0%)	710 (75.2%)	710 (61.6%)
≥65 years of age	1 (0.6%)	87 (9.2%)	88 (7.8%)
Total	178 (100.1%)	944 (100.0%)	1122 (99.9%)
Sex at Birth			
Female	83 (46.6%)	550 (58.3%)	633 (56.4%)
Male	95 (53.4%)	394 (41.7%)	489 (43.6%)
Ethnicity			
Hispanic/Latino	108 (60.7%)	427 (45.2%)	535 (47.7%)
Not Hispanic/Latino	70 (39.3%)	517 (54.8%)	587 (52.3%)
Race			
American Indian or Alaskan Native	1 (0.6%)	2 (0.2%)	3 (0.3%)
Asian	0 (0.0%)	4 (0.4%)	4 (0.4%)
Black or African American	8 (4.5%)	145 (15.4%)	153 (13.6%)
Native Hawaiian/Pacific Islander	0 (0.0%)	0 (0.0%)	0 (0.0%)

Demographic	Subjects (by lay-user collection and testing (N=178)	Self-collecting and testing (N=944)	Overall (N=1122)
White	161 (90.4%)	730 (77.3%)	891 (79.4%)
Unknown/Prefer not to answer	0 (0.0%)	0 (0.0%)	0 (0.0%)
Other (Mixed race/biracial)	8 (4.5%)	63 (6.7%)	71 (6.3%)
<b>Total</b>	<b>178 (100.0%)</b>	<b>944 (100.0%)</b>	<b>1122 (100.0%)</b>

## ANALYTICAL PERFORMANCE

### ANALYTICAL SENSITIVITY: LIMIT OF DETECTION (LoD)

The LoD of the device was performed to determine the lowest detectable concentration of SARS-CoV-2, influenza A and influenza B at which at least 95% of all true positive replicates are consistently detected as positive. The LoD was assessed for each analyte in two parts, a preliminary range finding study, followed by a confirmatory LoD study. A preliminary LoD was determined by first testing serial ten-fold dilutions of live influenza A and B, and inactivated SARS-CoV-2 virus stocks diluted into pooled negative swab matrix (PNSM) or pooled nasal wash (PNW) in 3 replicates per dilution and confirmatory testing was conducted with 20 replicates. Single analyte virus dilutions (50  $\mu$ L/swab) were each spiked onto dry sterile swabs and tested per the IFU. The lowest concentration that generated  $\geq 95\%$  positive detection rate was set as the LoD concentration.

The LoD for the analytes is identical when analytes are co-spiked into the same sample. The results of LoD confirmation testing for each virus are summarized in Table 3a.

**Table 3a: LoD Confirmation for SARS-CoV-2, Flu A, and Flu B**

Analyte	Isolate/Lineage	Strain	LoD Concentration (TCID <sub>50</sub> /mL)	LoD Concentration (TCID <sub>50</sub> /swab)	#Positive/# Total	# device lots tested
SARS-CoV-2	USA-WA1/2020 (UV inactivated)	NA	3.95E+02	1.98E+01	20/20	1
	USA-WA1/2020 (Heat inactivated)	NA	3.09E+03	1.5E+02	60/60	3
	USA/COR-22-063113/2022 (BA.5, Omicron variant)	NA	1.09E+03	5.45E+01	58/60	3
Flu A	H3N2	Darwin/6/21	2.09E+02	1.05E+01	20/20	1
	H1N1	Victoria/4897/22	2.02E+02	1.01E+01	20/20	1
		A/California/07/2009 pdm09	1.05E+03	5.25	60/60	3
		Guangdong-Maonan/SWL 1536/19 (PROtrol)	5.62E+01	2.81	60/60	3

Analyte	Isolate/Lineage	Strain	LoD Concentration (TCID <sub>50</sub> /mL)	LoD Concentration (TCID <sub>50</sub> /swab)	#Positive/# Total	# device lots tested
Flu B		inactivated)				
	Yamagata	Florida/04/06	1.46E+01	7.30E-01	20/20	1
	Victoria	Washington/02/19	1.58E+03	7.90E+01	20/20	1
	Victoria	Washington/02/19 (PROtrol inactivated)	1.75E+04	8.75E+02	58/60	3
	Victoria	B/Florida/78/2015	1.7E+04	8.5E+02	60/60	3

The First WHO International Standard for SARS-CoV-2 Antigen (NIBSC 21/368) was also tested in a similar manner to determine the LoD of SARS-CoV-2 antigen and the results are included in Table 3b.

**Table 3b: WHO SARS-CoV2 Standard Antigen LoD**

Description	Source	NIBSC. No.	Dilution Factor	Concentration (IU/ mL)	Concentration (IU/swab)
WHO International Standard SARS-CoV-2 Ag	NIBSC	21/368	1:80	250	12.5

### INCLUSIVITY (IN SILICO & ANALYTICAL SENSITIVITY)

Inclusivity testing was conducted to determine the analytical reactivity of the device with different strains of SARS-CoV-2, Flu A and Flu B.

A selection of temporal, geographic and genetically diverse Influenza A and B strains and SARS-CoV-2 were tested on the Healgen<sup>®</sup> Rapid Check<sup>®</sup> COVID-19/Flu A&B Antigen Test for inclusivity. Each strain was tested for reactivity in a dilution series and the lowest dilution in which 100% of replicates detected is included in Table 4.

**Table 4: Inclusivity Summary – Lowest Concentrations Tested Positive for Relevant Virus Strains**

Virus	Virus Strains	Concentration	Units	#positive/#tested
Flu A - H1N1	A/ California/04/2009	2.80E+03	TCID <sub>50</sub> /mL	3/3
	A/ Brisbane/02/2018	1.51E+02	TCID <sub>50</sub> /mL	3/3
	A/ Michigan/45/2015	9.30E+00	TCID <sub>50</sub> /mL	3/3
	A/ Guangdong-Maonan/SWL	1.04E+03	TCID <sub>50</sub> /mL	3/3
	A/ NY/03/2009	2.29E+04	TCID <sub>50</sub> /mL	3/3
	A/ Indiana/02/2020	9.70E+06	CEID <sub>50</sub> /mL	3/3
	A/Wisconsin/588/2019	1.4E+04	FFU/mL	3/3
	A/ Sydney/5/2021	4.80E+03	TCID <sub>50</sub> /mL	3/3
	A/ Hawaii/66/2019	3.70E+07	CEID <sub>50</sub> /mL	3/3
Flu A – H3N2	A/ Wisconsin/67/2022	1.05E+03	TCID <sub>50</sub> /mL	3/3
	A/New York/21/2020	2.6E+05	FFU/mL	3/3
	A/Tasmania/503/2020	6.5E+04	FFU/mL	3/3
	A/Hong Kong/2671/2019	3.1E+06	CEID <sub>50</sub> /mL	3/3
	A/Hong Kong/45/2019	1.5E+04	FFU/mL	3/3
	A/ Alaska/01/2021	1.50E+04	FFU/mL	3/3

Virus	Virus Strains	Concentration	Units	#positive/#tested
	A/Indiana/08/2011	8.10E+02	TCID <sub>50</sub> /mL	3/3
Flu A- H1N1	A/Ohio/09/2015	7.0E+05	CEID <sub>50</sub> /mL	3/3
Flu A- H1N2	A/Minnesota/19/2011	8.00E+06	CEID <sub>50</sub> /mL	3/3
Flu A- H5N1	A/mallard /Wisconsin/2576/2009	2.10E+05	GE/mL	3/3
	A/mallard/Wisconsin/2576/2009 (live)	800,000	CEID <sub>50</sub> /mL	3/3
	A/Bovine/Ohio/B24OSU-439/2024	1,550	TCID <sub>50</sub> /mL	3/3
	A/duck/Guangxi/S11002/2024	3.38E+05	EID <sub>50</sub> /mL	5/5
Flu A- H5N6	A/duck/Guangxi/S10888/2024	7.90E+05	EID <sub>50</sub> /mL	5/5
Flu A- H5N8	A/goose/Liaoning/S1266/2021	1.69E+05	EID <sub>50</sub> /mL	5/5
Flu A- H7N3	A/northern pintail/Illinois/10OS3959/2010	7.0E+05	CEID <sub>50</sub> /mL	3/3
Flu B – Victoria Lineage	B/ Brisbane/60/2008	6.45E-01	TCID <sub>50</sub> /mL	3/3
	B/Colorado/6/2017	5.85E+00	TCID <sub>50</sub> /mL	3/3
	B/Texas/02/2013	6.13E+00	TCID <sub>50</sub> /mL	3/3
	B/ Michigan/01/2021	2.85E+03	TCID <sub>50</sub> /mL	3/3
Flu B – Yamagata Lineage	B/Texas/06/2011	8.00E+05	CEID <sub>50</sub> /mL	3/3
	B/Utah/09/2014	1.26E+02	TCID <sub>50</sub> /mL	3/3
	B/Wisconsin/1/10	1.78E+01	TCID <sub>50</sub> /mL	3/3
Flu B – non-Victoria, non-Yamagata	B/Maryland/1/1959	1.69E+03	CEID <sub>50</sub> /mL	3/3
SARS-CoV-2 Delta	B.1.617.2	2.82E+5	genome copies/mL	3/3
SARS-CoV-2 Beta	B.1.351	2.12E+5	genome copies/mL	3/3
SARS-CoV-2 Alpha	B.1.1.7	6.48E+5	genome copies/mL	3/3
SARS-CoV-2 Omicron	B.1.1.529	2.51E+2	TCID <sub>50</sub> /mL	3/3
SARS-CoV-2 Gamma	P1	6.30E+2	TCID <sub>50</sub> /mL	3/3
SARS-CoV-2 Kappa	B.1.617.1	1.90E+2	TCID <sub>50</sub> /mL	3/3
SARS-CoV-2 Omicron	JN1*	26.4	Ct Values	5/5

\*The pooled JN1 positive clinical sample was provided by and tested at Emory using the Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test for reactivity in a dilution series. All five replicates at mean ≤ 26.4 were tested positive.

#### HOOK EFFECT

The hook effect study was conducted to evaluate if high levels of antigen present in the sample could result in a false negative test result. In this study, 50 µL of the highest concentration possible of UV inactivated SARS-CoV-2 virus stock, each of the live Influenza A virus stock, H1N1 pdm09 and H3N2, and each live Influenza B virus stock, Victoria and Yamagata, were spiked onto the sterile swab and tested in triplicate on the Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test to test for a high-dose hook effect. The Healgen®

Rapid Check® COVID-19/Flu A&B Antigen Test showed no hook effect for SARS-CoV-2, Flu A, and Flu B, at the concentrations listed in Table 5.

Table 5: Summary of Hook Effect

Virus	Subtype or Lineage	Concentration without Hook Effect	
		(TCID <sub>50</sub> /mL)	(TCID <sub>50</sub> /swab)
SARS-CoV-2	N/A	3.16E+06	1.58E+05
Influenza A	H1N1	2.02E+05	1.01E+04
Influenza A	H3N2	4.17E+05	2.09E+04
Influenza B	Victoria	3.16E+06	1.58E+05
Influenza B	Yamagata	1.17E+05	5.85E+03

#### ANALYTICAL SPECIFICITY: CROSS REACTIVITY (EXCLUSIVITY) AND MICROBIAL INTERFERENCE

The analytical specificity/interference of the Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test was evaluated by testing various commensals and pathogenic microorganisms in the absence (cross-reactivity) and presence (microbial interference) of SARS-CoV-2/Flu A/Flu B at 3x LoD. Each organism was tested in replicates of three (3) with or without SARS-CoV-2/FluA/FluB present in the sample. No cross-reactivity and no microbial interference was observed for any of the listed organisms when tested in the concentrations listed in Table 6.

Table 6: Summary of Cross-reactivity and Microbial Interference

ID	Organism	Concentration tested	Units	Cross-reactivity	Microbial Interference
SARS	SARS-CoV-1	1.25E+05	PFU/mL	ND*	ND
MERS	MERS-coronavirus	1.47E+05	TCID <sub>50</sub> /mL	ND	ND
OC43	Human coronavirus OC43	7.00E+05	TCID <sub>50</sub> /mL	ND	ND
229E	Human coronavirus 229E	1.58E+05	TCID <sub>50</sub> /mL	ND	ND
NL63	Human coronavirus NL63	8.00E+04	TCID <sub>50</sub> /mL	ND	ND
AV1	Adenovirus, Type 1 (Adenoid 71)	2.23E+05	TCID <sub>50</sub> /mL	ND	ND
AV7	Adenovirus Type 7, Type 7A (Species B)	1.58E+05	TCID <sub>50</sub> /mL	ND	ND
CMV	Cytomegalovirus, Strain AD-169	7.05E+04	TCID <sub>50</sub> /mL	ND	ND
EBV	Epstein Barr Virus, Strain B95-8	1.83E+06	CP/mL	ND	ND
hMPV	Human Metapneumovirus (hMPV), Strain TN/91-316	3.50E+05	TCID <sub>50</sub> /mL	ND	ND
P1	Parainfluenza virus 1, Strain ERA/2922/1106/2009	2.00E+05	TCID <sub>50</sub> /mL	ND	ND
P2	Parainfluenza virus 2, Strain Greer	1.75E+05	TCID <sub>50</sub> /mL	ND	ND
P3	Parainfluenza virus 3, Strain C243	7.00E+05	TCID <sub>50</sub> /mL	ND	ND
P4	Parainfluenza virus 4, Strain N/A	2.39E+05	TCID <sub>50</sub> /mL	ND	ND
EV68	Enterovirus Type (e.g. 68), Species D Type 68	2.23E+05	TCID <sub>50</sub> /mL	ND	ND
RSVA	Respiratory syncytial virus A, Strain A-2	3.50E+05	TCID <sub>50</sub> /mL	ND	ND
RSVB	Respiratory syncytial virus B, Strain CH93(18)-18	2.29E+05	TCID <sub>50</sub> /mL	ND	ND
RV	Rhinovirus 1A, Strain N/A	7.05E+04	TCID <sub>50</sub> /mL	ND	ND

ID	Organism	Concentration tested	Units	Cross-reactivity	Microbial Interference
BP	Bordetella pertussis, Strain A639	2.50E+08	CFU/mL	ND	ND
CA	Candida albicans, Strain Z006	6.03E+06	CFU/mL	ND	ND
CP	Chlamydia pneumoniae, Strain Z500	4.33E+06	IFU/mL	ND	ND
CB	Corynebacterium xerosis	2.30E+07	CFU/mL	ND	ND
EC	Escherichia coli, Strain mcr-1	1.79E+08	CFU/mL	ND	ND
HI	Hemophilus influenzae, type b; Eagan	9.68E+06	CFU/mL	ND	ND
LB	Lactobacillus sp., Lactobacillus Acidophilus, Strain Z048	1.21E+07	CFU/mL	ND	ND
LP	Legionella spp pneumophila, Strain Philadelphia-1	6.50E+06	CFU/mL	ND	ND
MC	Moraxella catarrhalis, Strain 59632	2.50E+08	CFU/mL	ND	ND
MP	Mycoplasma pneumoniae, Strain PI 1428	2.50E+07	CFU/mL	ND	ND
MT	Mycobacterium tuberculosis avirulent, Strain	4.15E+06	CFU/mL	ND	ND
NM	Neisseria meningitidis, serogroup A	3.43E+06	CFU/mL	ND	ND
NS	Neisseria sp. Elongata Z071	2.68E+08	CFU/mL	ND	ND
PJ	Pneumocystis jirovecii, Strain W303-Pji	1.30E+07	CFU/mL	ND	ND
PA	Pseudomonas aeruginosa, Strain N/A	3.45E+08	CFU/mL	ND	ND
SA	Staphylococcus aureus Protein A producer, e.g., Cowan strain, NCTC 8530 [S11]; Cowan's serotype 1	2.60E+08	CFU/mL	ND	ND
SE	Staphylococcus epidermidis (PCI 1200)	9.00E+07	CFU/mL	ND	ND
SS	Streptococcus salivarius, Strain C699 [S30D]	1.01E+06	CFU/mL	ND	ND
SPN	Streptococcus pneumoniae, Strain Z022	1.81E+07	CFU/mL	ND	ND
SPY	Streptococcus pyogenes, Strain MGAS 8232	7.50E+07	CFU/mL	ND	ND
ME	Measles, Strain Edmonston	8.48E+05	TCID <sub>50</sub> /mL	ND	ND
MU	Mumps (Isolate 1)	8.48E+05	TCID <sub>50</sub> /mL	ND	ND
HKU1 <sup>a</sup>	Human coronavirus HKU1	1:20	-	-	ND

\*ND: Not Detected.

<sup>a</sup>1:10 dilution of cultured stock HKU1 sample from Emory

#### COMPETITIVE INTERFERENCE

Competitive interference of the test's analytes was tested with different combinations of low (3x LoD) and high concentrations of Flu A, Flu B and SARS-CoV-2 spiked together onto a swab and then tested with one lot of Healgen® Rapid Check® COVID-19/Flu A&B Antigen test device strains to determine if the assay can detect target analytes across a variety of analyte concentration combinations. All testing conditions have been tested in 3 replicates. The study used inactivated SARS-CoV-2 but live influenza A and B virus. The Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test showed no competitive interference from the analytes co-existed in the specimens at the concentrations indicated in Table 7.

Table 7: Competitive Interference Results

	Analyte Concentration Added to Sample* (# of positive replicates / # of total replicates)		
	Flu A	Flu B	SARS-CoV-2
Analyte Concentration Added Results	667X LoD 3/3	3X LoD 3/3	- 0/3
Analyte Concentration Added Results	667X LoD 3/3	- 0/3	3X LoD 3/3
Analyte Concentration Added Results	3X LoD 3/3	2667X LoD 3/3	- 0/3
Analyte Concentration Added Results	- 0/3	2667X LoD 3/3	3X LoD 3/3
Analyte Concentration Added Results	3X LoD 3/3	- 0/3	2667X LoD 3/3
Analyte Concentration Added Results	- 0/3	3X LoD 3/3	2667X LoD 3/3

\* SARS-CoV-2 strain – 1X LoD - 3.95E+02 TCID<sub>50</sub>/mL

Flu A – H3N2:A/Darwin/6/2021 – 1X LoD – 2.09E+02 TCID<sub>50</sub>/mL

Flu B – Yamagata: B/Florida/4/2006 – 1X LoD - 1.46E+01 TCID<sub>50</sub>/mL

#### INTERFERING SUBSTANCES

The Healgen® Rapid Check® COVID-19/Flu A&B Antigen test was evaluated for performance in the presence and absence of potentially interfering substances that might be present in a respiratory specimen at concentrations listed in the below table. Negative specimens were evaluated in triplicates to confirm that the potentially interfering substances would not cause false positive results with the test. Substances that did not cause a false-positive result was further evaluated for interference by testing substance spiked negative clinical matrix mixed 1:1 with co-spiked (with SARS-CoV-2/Flu A/Flu B virus) negative clinical matrix to achieve a final virus concentration of 3X single analyte LoD and tested in triplicate. If interference was observed at the level tested, an additional titration study would have been performed to determine the highest interfering substance level the Healgen multiplex test can tolerate.

With the exception of Flu Mist Quadrivalent live influenza vaccine, none of the substances caused a false-positive test result in unspiked samples. While the presence of Flu Mist Quadrivalent live influenza vaccine at 15% v/v concentration did not interfere with the detection of true positive results of the 3x LoD co-spiked samples, the vaccine also resulted in positive results for Flu A and Flu B (as expected based on the composition of the vaccine). When diluted down to 0.15% v/v, the results of the unspiked samples were negative. Hand sanitizer cream lotion and hand sanitizer 80% ethanol fast drying at 15% v/v showed false negative results for Flu B, but detected all analytes at 7.5% v/v.

The interfering substances test results are shown in Table 8.

Table 8: Potential Interfering Substances

Interfering Substance	Concentra-tion	Cross-reactivity (no analyte) (# pos/ # total)			Interference (3x co-spiked analyte LoD) (# pos/ # total)		
		SARS-CoV-2	Flu A	Flu B	SARS-CoV-2	Flu A	Flu B
Human Whole Blood (EDTA tube)	4% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Leukocytes	1.67 x 10 <sup>6</sup> cells/mL	0/3	0/3	0/3	3/3	3/3	3/3
Throat Lozenges (Menthol/Benzocaine)	3 mg/mL	0/3	0/3	0/3	3/3	3/3	3/3
Mucin, bovine submaxillary gland	2.5 mg/mL	0/3	0/3	0/3	3/3	3/3	3/3
Zinc (Therazinc throat Spray)	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Naso GEL (NeilMed)	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Nasal Drops (Phenylephrine)	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Nasal Spray (Oxymetazoline)	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Nasal Spray (Cromolyn)	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Nasal Corticosteroid (Dexamethasone)	1 mg/mL	0/3	0/3	0/3	3/3	3/3	3/3
Nasal Corticosteroid (Fluticasone Propionate)	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Nasal gel (Galphimia glauca, Histanium hydrochloricum, Luffa operculata, Sulfur)	1.25%	0/3	0/3	0/3	3/3	3/3	3/3
Homeopathic allergy relief (Histaminum hydrochloricum)	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Zicam nasal spray (Galphimia glauca, Luffa operculata)	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Nasal spray (Alkalol)	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Sore Throat Phenol Spray	15% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Tobramycin	4 µg/mL	0/3	0/3	0/3	3/3	3/3	3/3
Mupirocin	10 mg/mL	0/3	0/3	0/3	3/3	3/3	3/3
Anti-viral drug (Remdesvir)	10 mg/mL	0/3	0/3	0/3	3/3	3/3	3/3
Tamiflu (Oseltamivir)	5 mg/mL	0/3	0/3	0/3	3/3	3/3	3/3
FluMist (Quadrivalent/Live)	15% v/v	0/3	3/3	3/3	3/3	3/3	3/3
	0.15% v/v	0/3	0/3	0/3	NA	NA	NA
Zanamivir	282 ng/mL	0/3	0/3	0/3	3/3	3/3	3/3
Biotin	3500 ng/mL	0/3	0/3	0/3	3/3	3/3	3/3
Body & Hand Lotion	0.5% w/v	0/3	0/3	0/3	3/3	3/3	3/3
Body Lotion, with 1.2% dimethicone	0.5% w/v	0/3	0/3	0/3	3/3	3/3	3/3
Hand Lotion	5% w/v	0/3	0/3	0/3	3/3	3/3	3/3
Hand Sanitizer with Aloe, 62% ethyl alcohol	5% w/v	0/3	0/3	0/3	3/3	3/3	3/3
Hand Sanitizer cream lotion	15% v/v	0/3	0/3	0/3	3/3	3/3	0/3
	7.5% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Hand Sanitizer, 80% ethanol	15% v/v	0/3	0/3	0/3	3/3	3/3	0/3
	7.5% v/v	0/3	0/3	0/3	3/3	3/3	3/3
Hand soap	10% w/v	0/3	0/3	0/3	3/3	3/3	3/3

Interfering Substance	Concentra-tion	Cross-reactivity (no analyte) (# pos/ # total)			Interference (3x co-spiked analyte LoD) (# pos/ # total)		
		SARS-CoV-2	Flu A	Flu B	SARS-CoV-2	Flu A	Flu B
liquid gel							

#### PRECISION

The Precision study for the Healgen® Rapid Check® COVID-19/Flu A&B Antigen Test was evaluated in two different in-house studies using the same 3 lots of test kits and the same operators.

Study 1 was conducted by 2 trained operators. Three sample levels (2X LoD co-spiked, 5X LoD co-spiked and Negative Pooled Nasal Wash) were tested on each day, one replicate per run, per operator, and per lot of devices. Two (2) runs (morning and afternoon) were conducted each day per operator, per lot, per day. This exact testing scheme was carried out over 10 days (same 3 sample levels tested, on the same 3 lots, by the same 2 operators, in 2 runs per day). This resulted in 120 total tests per sample level. All samples were randomized and blinded for each day. For all three lots and operators, the results for this study shown in the table below were identical and concordant with the expected results.

Study 2 was specifically conducted to further evaluate potential differences between lots. The study used negative samples (without virus analytes) and very low positive samples at 0.75x LoD, commonly referred to as high negative sample. Samples were prepared near the C95 concentration for all three analytes and were randomized and blinded. This supplemental precision testing was carried out over 3 days only, but otherwise followed the same study design as above. This resulted in 72 total tests per analyte and sample level (24 replicates for each analyte with each lot). Data from this testing are integrated into Table 9 below.

Table 9: Summary of Precision Results

Sample	Analyt-e	Lot 1		Lot 2		Lot 3		Total Percent Lot-to-Lot Agree-ment	95% CI
		Count*	% Agreement	Count*	% Agreement	Count*	% Agreement		
Negative	SARS-CoV-2	0/64	100%	0/64	100%	0/64	100%	100%	98.0-100%
	Flu A	0/64	100%	0/64	100%	0/64	100%	100%	98.0-100%
	Flu B	0/64	100%	0/64	100%	0/64	100%	100%	98.0-100%
0.75 x LoD	SARS-CoV-2	20/24	83.3%	22/24	91.7%	17/24	70.8%	81.9%	71.5-89.1%
	Flu A	15/24	62.5%	15/24	62.5%	15/24	62.5%	62.5%	50.9-72.8%
	Flu B	18/24	75.0%	17/24	70.8%	14/24	58.3%	68.0%	56.6-76.7%
2 x LoD	SARS-CoV-2	40/40	100%	40/40	100%	40/40	100%	100%	93.9-100%
	Flu A	40/40	100%	40/40	100%	40/40	100%	100%	93.9-100%
	Flu B	40/40	100%	40/40	100%	40/40	100%	100%	93.9-100%
5 x LoD	SARS-CoV-2	40/40	100%	40/40	100%	40/40	100%	100%	93.9-100%
	Flu A	40/40	100%	40/40	100%	40/40	100%	100%	93.9-100%
	Flu B	40/40	100%	40/40	100%	40/40	100%	100%	93.9-100%

## REFERENCES

1. Julien Favresse, Constant Gillot, Maxime Oliveria, Julie Cadrobbi, Marc Elsen, Christine Eucher, Kim Laffineur, Catherine Rosseels, Sandrine Van Eeckhoudt, Jean-Baptiste Nicolas, Laure Moiremont, Jean-Michael Dogné and Jonathan Douxfils. Head-to-Head Comparison of Rapid and Automated Antigen Detection Tests for the Diagnosis of SARS- CoV-2 Infection J. Clin. Med. 2021, 10, 265.
2. Ignacio Torres, Sandrine Poujois, Eliseo Albert, Gabriela Álvarez, Javier Colomina and David Navarro. Point-of-care evaluation of a rapid antigen test for diagnosis of SARS- CoV-2 infection in symptomatic and asymptomatic individuals February 11, 2021
3. Moghadami M. A Narrative Review of Influenza: A Seasonal and Pandemic Disease. Iran J Med Sci. 2017

## SYMBOL INDEX

	Do not reuse		See Instruction for Use		Expiration Date
	Tests per Kit		Store Between 2-30°C (36-86°F)		Keep Dry
	Batch Number		Catalog#		Keep Away from Sunlight
	Unique Device Identifier		For <i>in vitro</i> diagnostic use only		Manufacturer
	Do not use if package is damaged				



Healgen Scientific, LLC.

Address: 3818 Fuqua Street, Houston, TX 77047

Toll-Free: +1 (866) 982-3818 (Monday - Friday 8:30 a.m to 5 p.m. CDT)

Customer Service: support@healgen.com

Website: www.healgen.com

Revision Date: 2024-10-16  
B23708-01